
Summary Report of IQC program for G6PD Quantitative Test - Medicon Group - November 2018 -


I. The statistic results of all laboratories in this month


G6PD	Control N (Lot No.:AE0909N)	Control D (Lot No.:AE0909D)
Labs	7	7
Received results number (n)	34	34
Median	14.9 (U/gHb)	5.3 (U/gHb)
Mean	14.5 (U/gHb)	5.3 (U/gHb)
SD	0.9	0.2
CV	6.2%	3.8%
Range of G6PD	$12.3 \sim 15.8 (\text{U/gHb})$	$4.8 \sim 5.7 (\text{U/gHb})$
Range of Hb	$1.7 \sim 2.2 \text{ (g/dL)}$	$2.0 \sim 2.4 \text{ (g/dL)}$

^{*}The statistic results are calculated from all labs reported in this month

II. The distribution of G6PD reported for each lab in this survey

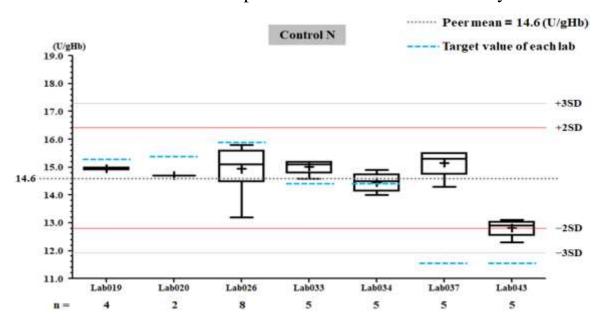



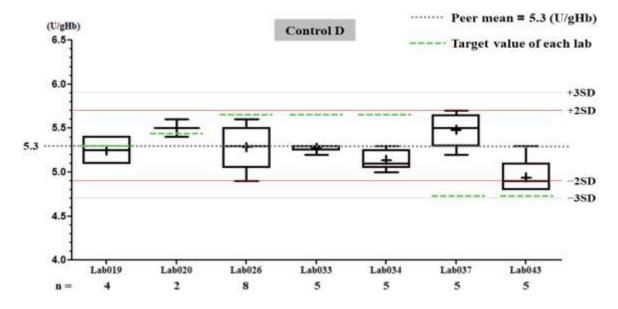



^{**} G6PD Method = Medicon reagent kit, 37°C